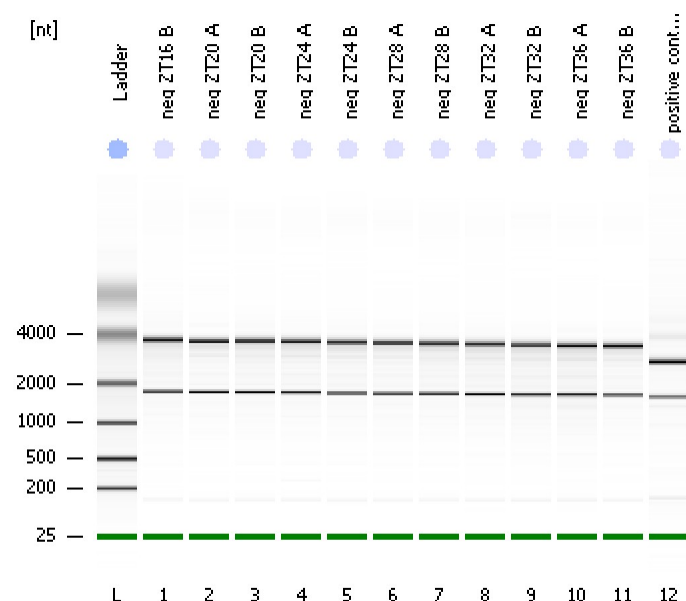


Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

Electrophoresis File Run Summary**Instrument Information:**













Instrument Name: Ann's baby
Serial#: DE24802235
Firmware: C.01.069
Type: G2938B

Assay Information:

Assay Origin Path: D:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Nano Series II.xsy
Assay Class: Eukaryote Total RNA Nano
Version: 2.6
Assay Comments: Total RNA Analysis ng sensitivity (Eukaryote)
© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

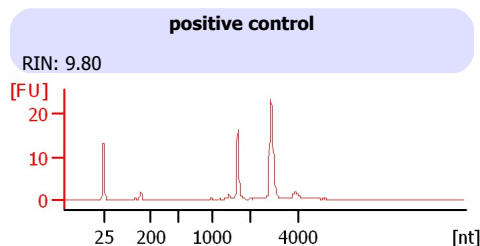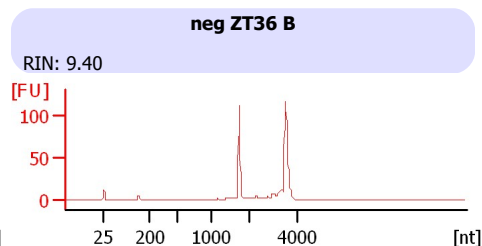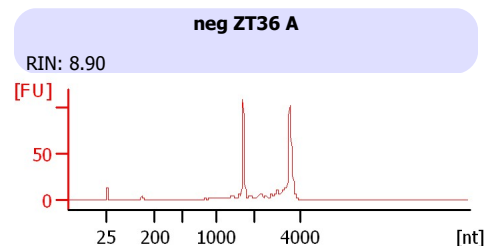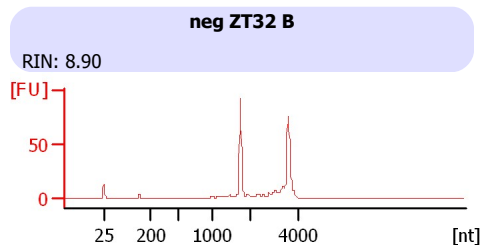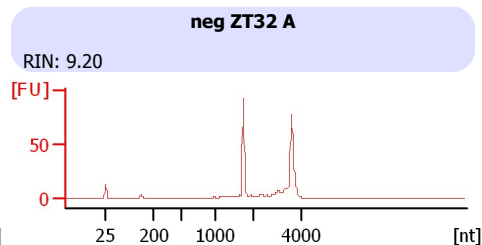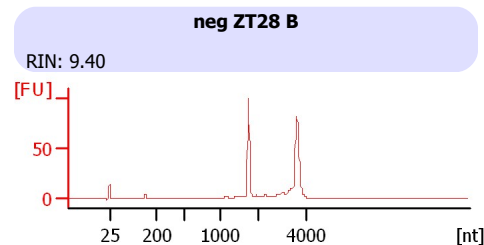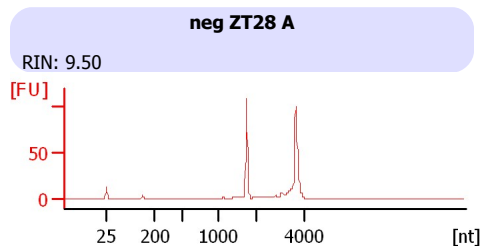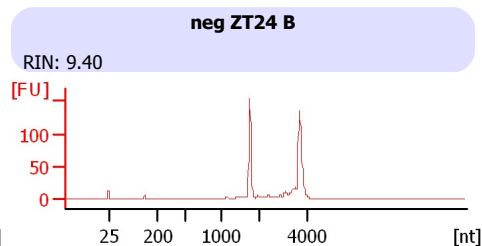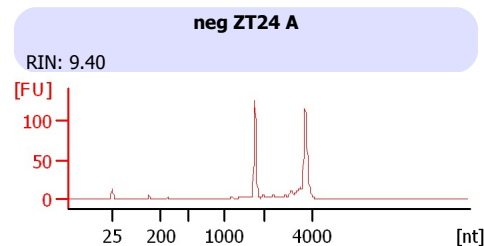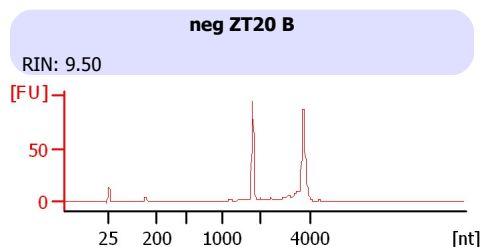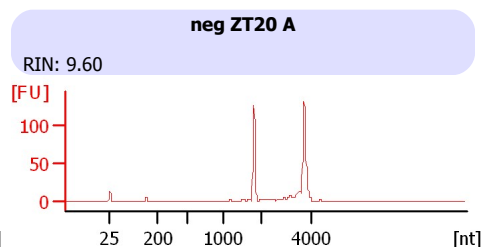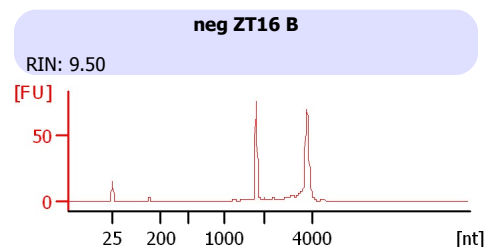

Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
neg ZT16 B		✓	RIN: 9.50	
neg ZT20 A		✓	RIN: 9.60	
neg ZT20 B		✓	RIN: 9.50	
neg ZT24 A		✓	RIN: 9.40	
neg ZT24 B		✓	RIN: 9.40	
neg ZT28 A		✓	RIN: 9.50	
neg ZT28 B		✓	RIN: 9.40	
neg ZT32 A		✓	RIN: 9.20	
neg ZT32 B		✓	RIN: 8.90	
neg ZT36 A		✓	RIN: 8.90	
neg ZT36 B		✓	RIN: 9.40	
positive control		✓	RIN: 9.80	
Ladder		✓	All Other Samples	

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 13

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 19

End Analysis Time Range [s] : 69

Ladder Concentration [ng/μl] : 150

Lower Marker Concentration [ng/μl] : 0

Upper Marker Concentration [ng/μl] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 19

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.5

Area Threshold : 0.2

Width Threshold [s] : 0.5

Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad





Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

Electropherogram Summary

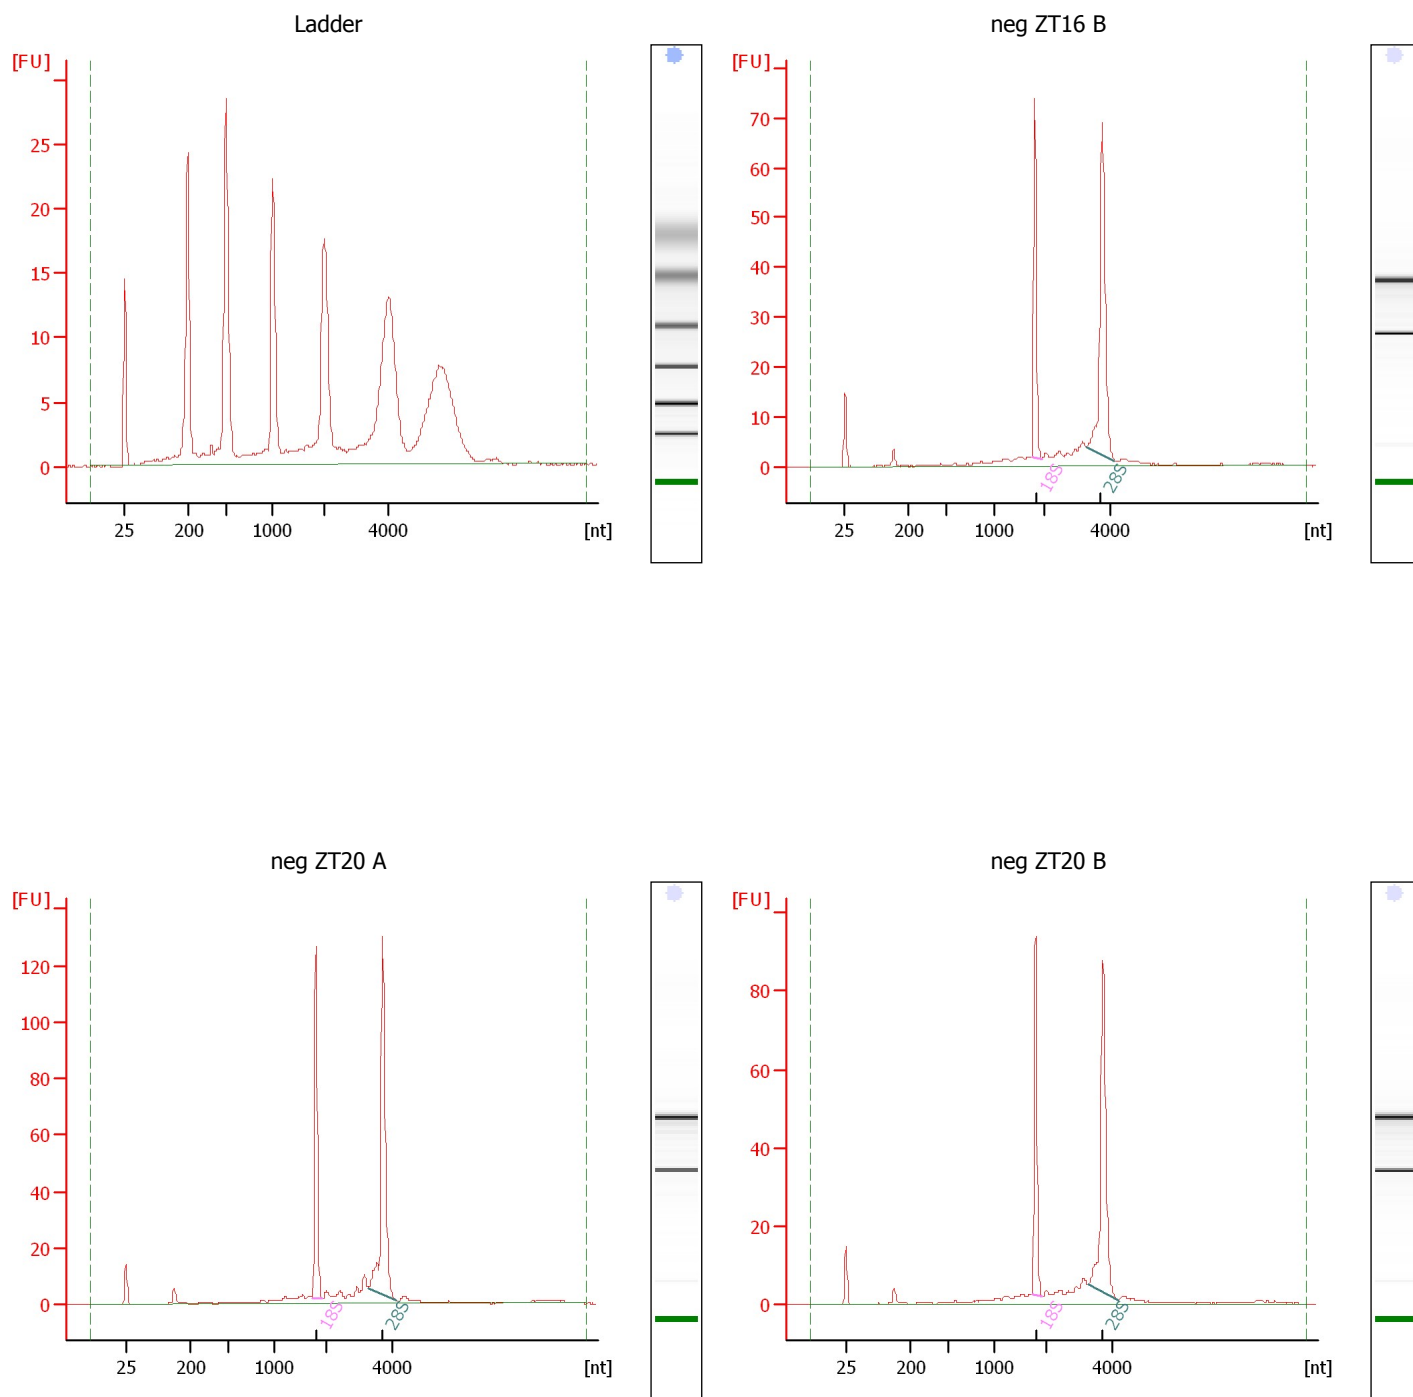


Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...\Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

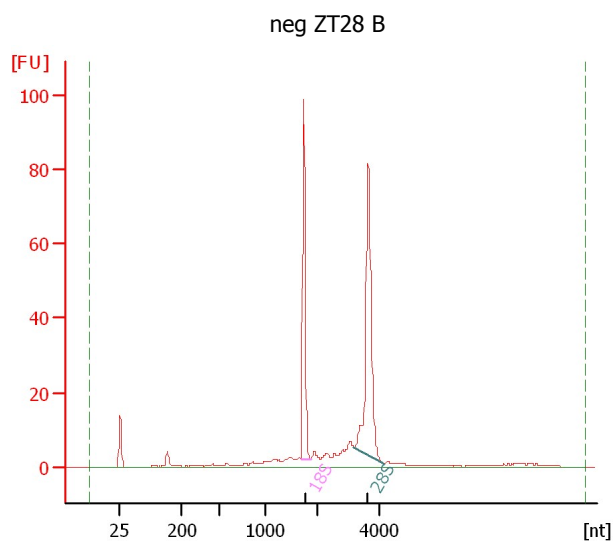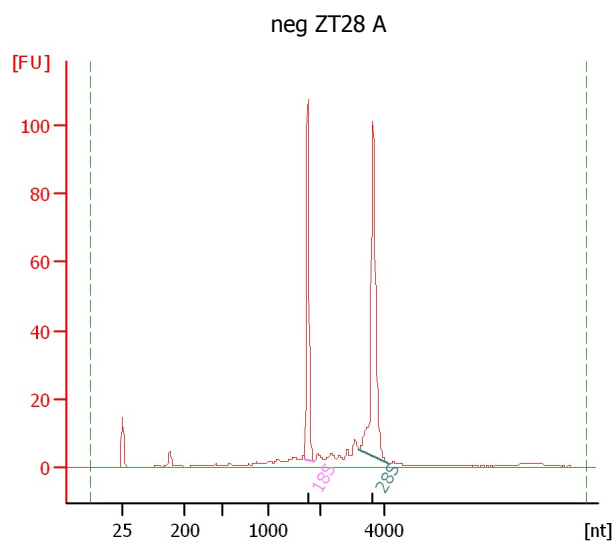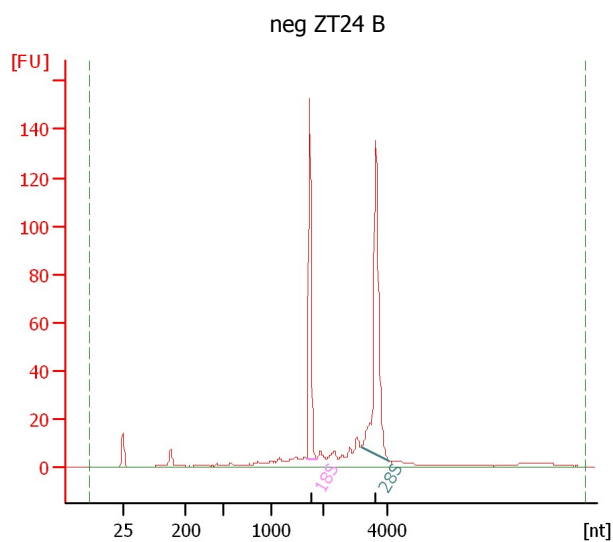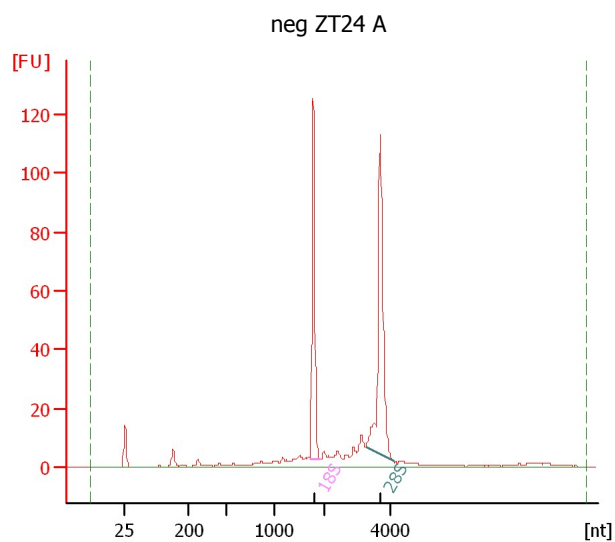Electropherogram Summary Continued ...


Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

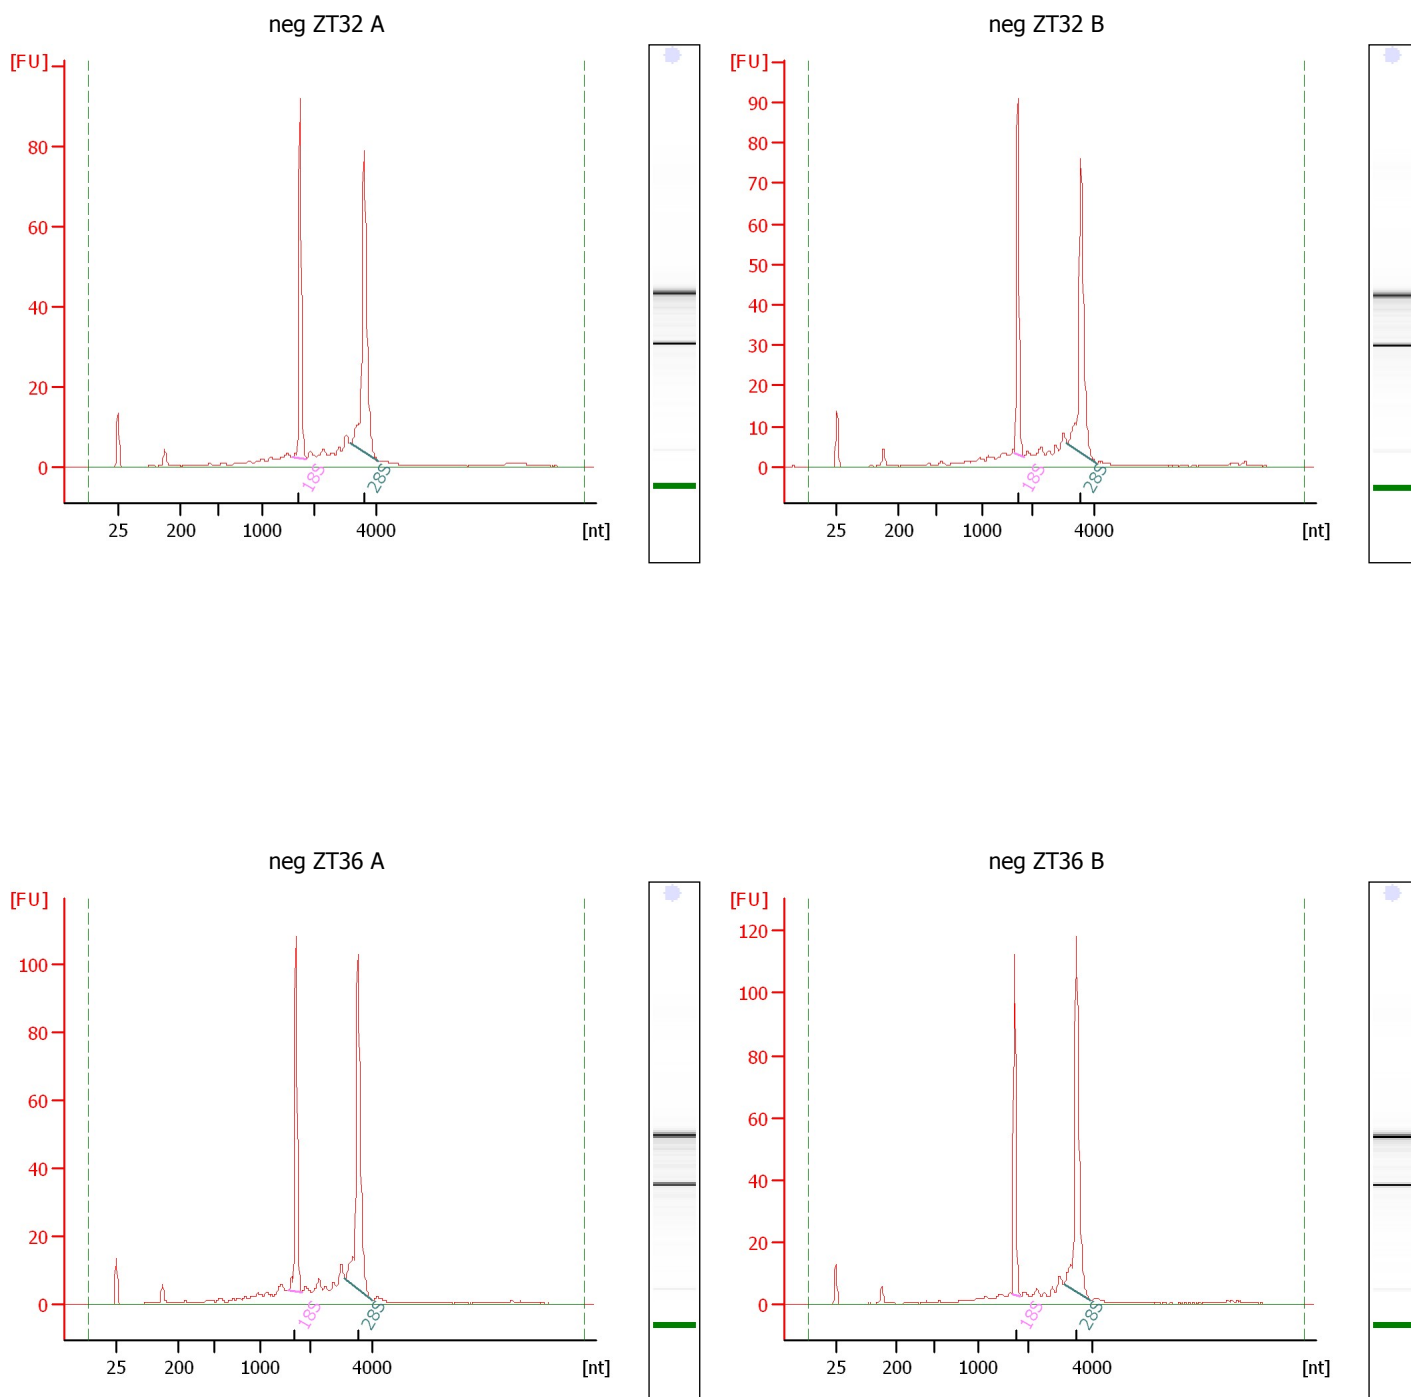Electropherogram Summary Continued ...

Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

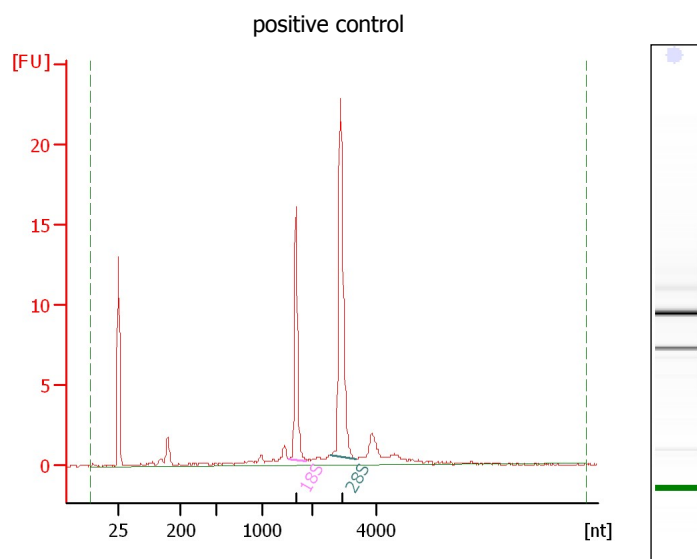Electropherogram Summary Continued ...

Assay Class: Eukaryote Total RNA Nano
Data Path: D:\...Eukaryote Total RNA Nano_DE24802235_2012-03-28_16-58-03.xad

Created: 3/28/2012 4:58:02 PM
Modified: 3/28/2012 5:21:13 PM

Gel Image